

## Reaction Screening Using a Microreactor

Olivier Naef<sup>\*</sup>, Mathieu Roch, and Thierry Chappuis

<sup>\*</sup>Correspondence: Prof. O. Naef, Ecole d'ingénieurs et d'architectes de Fribourg  
Boulevard de Pérolles 80, CP 32, CH-1705 Fribourg, Tel.: +41 26 429 67 05  
E-mail: olivier.naef@hefr.ch

**Abstract:** This article discusses the screening of chemical reactions using a microreactor equipped with infrared spectroscopy as online analytics. An esterification reaction has been optimized in continuous mode with the proposed setup. The esterification did not work well due to the material of the microreactor (stainless-steel 316Ti) that catalyzed the decomposition of formic acid. However, despite the occurrence of decomposition, an optimization could be achieved with this system.

**Keywords:** Continuous mode · Esterification · Microreactor · Optimization · Screening


## 1. Introduction

Our world has limited resources and a population that continually increases. Sustainable development is the main key to success for the future in the 21st century. Chemistry must play a central role in this process. In this context, only optimized chemical processes which have reached a maximum efficiency will lead to more sustainable products and production. Developing new chemicals implies, in an early step, an analysis of different parameters to be used during the optimization phase. A fundamental challenge in organic chemistry is to understand the reaction mechanism. In order to obtain this information, the chemical kinetics, including the reaction order and the rate constants, must be determined through experimentation.


The determination of the reaction mechanism requires intensive testing in the laboratory. Today, the chemist often uses an automated parallel system to collect data. The fed-batch mode is most often chosen to carry out the reaction. Its advantage is the flexibility during the introduction of the reactants and the possibility to work with solids, liquids or gases. The transfer from a fed-batch process to continuous mode is often difficult. Nevertheless the continuous mode has numerous advantages over fed-batch such as the possibility to work under steady-state conditions. This results in the possibility to adapt and control parameters, which facilitates the extraction of useful information. Using a tubular continuous microreactor with a small volume, a high heat transfer capacity and advanced automation possibilities presents significant benefits. Efficient screening of chemical reactions using fed-batch or continuous processes attempts to minimize:

- manpower,
- contact of laboratory personnel with chemicals,
- screening time, and
- quantity of chemicals used.

The use of a fully-automated microreactor<sup>[1]</sup> equipped with online analytics and software specifically designed for screening of chemical reactions should provide answers to these ques-

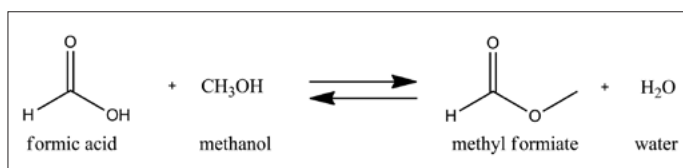

Scheme 1. Esterification reaction between formic acid and methanol.

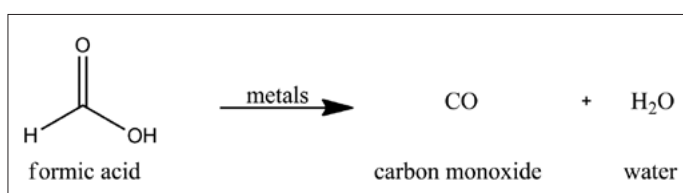

Scheme 2. Probable decomposition reaction of formic acid in presence of metals.

tions. This paper is based on the Bachelor thesis of Mathieu Roch.<sup>[2]</sup>

## 2. Reaction

Scheme 1 shows the esterification reaction between formic acid and methanol, producing methyl formate and water, as tested by Droz.<sup>[3]</sup> In a typical case (fed-batch process), the water is distilled off during the reaction to move the equilibrium to the right. In the present case, due to the use of a microreactor made of stainless steel, the potential metal-catalyzed decomposition of formic acid must be considered. Scheme 2 presents this decomposition to produce water and carbon monoxide.

## 3. Experiment Setup

The setup presented in Fig. 1 can be divided into three main parts: the pumps, the microreactor, and the infrared spectrophotometer.

Two different pumping systems have been used with this installation. The first system was formed by two MZR 7208X1 S pumps from LEWA able to work in a range from 0.048 to 288 ml/min. The second system is made with two Encore™ HPLC pumps from Zymark functioning between 0.1 and 5 ml/min. The exact added mass was measured with two lab balances (Mettler-Toledo GmbH PR5002) placed upstream.

The microreactor used in the present study is an Ehrfeld system (Ehrfeld Mikrotechnik BTS, Wendelsheim, Germany) formed of an A3 clamping device, a slit plate mixer LH 25 (655 µl) with a temperature sensor, a Meander reactor (11.3 ml) thermostated with a Julabo oil bath (20 °C to 100 °C), a coaxial heat exchanger (620 µl) also connected to a second Julabo MV oil bath, and connection modules from Ehrfeld and from the Swagelok company.

The infrared spectra are realized with a PerkinElmer Spectrum 100 FTIR spectrophotometer including an ATR probe (Pike

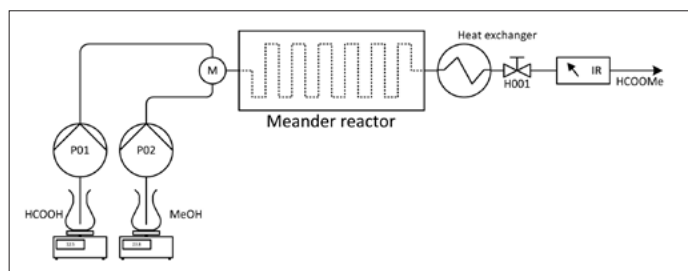


Fig. 1. Scheme of the microreactor used including the two pumps, the mixer, the Meander reactor, the heat exchanger, and the infrared spectrophotometer.

GladiATR) and a flow cell. A Mettler-Toledo React-IR can also be connected to this setup through a homemade flow cell.

#### 4. Screening Methodology

In order to analyze the kinetics of the reaction, the concentration of the species at different times must be measured. With the reaction being carried out in a continuous tubular microreactor (assumption of a plug flow reactor – Reynolds number below 1'500), the flow rate of each pump can be modified to obtain different residence times. The concentration profile in the out-flow as a function of the residence time can then be compared to the concentration profile of the same reaction implemented in a batch reactor. One possibility in order to use such a tubular microreactor to screen conditions is to test systematically a large set of feasible flow rates in the range allowed by the setup. Another option is to use a design of experiments strategy. The second method has been used in the present study, based on a Central Composite Face-centered (CCF) experimental design.<sup>[4]</sup> The CCF design, for three parameters, can be represented by a cube. The parameters are chosen on the extremes of the cube edge (corresponding to the maxima and minima of each parameter), at the center of each side, and at the middle of the cube. This method can be used not only for the determination of kinetic parameters but also to achieve a reaction optimization (yield and selectivity). The design of experiments strategy can also be used to analyze the correlation between the parameters.

Infrared spectroscopy was used to retrieve the concentration of the species for the esterification reaction. The Beer-Lambert law described for example by Stuart,<sup>[5]</sup> applied to the spectral information (matrix **D**), approximates the spectrum to a linear combination of the pure infrared spectra (matrix **S**) multiplied by the molar concentration (matrix **C**).

$$\mathbf{D} = \mathbf{C} \cdot \mathbf{S}^T$$

Using multiple linear regression (MLR),<sup>[6]</sup> the estimated concentration **C** can be retrieved by setting the error (**E**) to **0**. This estimation corresponds to a multiplication of the data matrix (**D**) by the pseudo-inverse matrix of the pure infrared spectra (**S**).

$$\mathbf{C} = \mathbf{D} \cdot (\mathbf{S}^T)^+$$

Advanced chemometric methods<sup>[7]</sup> give more robustness in the concentration estimation. The Multivariate Curves Resolution (MCR)<sup>[8]</sup> is implemented in our screening technique.

In order to study the kinetic behavior of the reaction, a kinetic model was implemented. With the assumptions that the tubular

microreactor can be represented by a perfect plug flow reactor and that the mixture is in a single phase with a constant heat capacity ( $c_p$ ) and density ( $\rho$ ) and in isothermal conditions, the model is given by the partial mass balances for each species. As an example, for the esterification reaction of formic acid and methanol to methyl formiate and water,<sup>[9]</sup> the model is based on the following system of five differential equations.

$$\begin{aligned} u \cdot \frac{d[\text{HCOOH}]}{dz} &= -k_1 \cdot [\text{HCOOH}] \cdot [\text{MeOH}] + k_{-1} \cdot [\text{H}_2\text{O}] \cdot [\text{HCOOMe}] - k_2 \cdot [\text{HCOOH}] \\ u \cdot \frac{d[\text{MeOH}]}{dz} &= -k_1 \cdot [\text{HCOOH}] \cdot [\text{MeOH}] + k_{-1} \cdot [\text{H}_2\text{O}] \cdot [\text{HCOOMe}] \\ u \cdot \frac{d[\text{H}_2\text{O}]}{dz} &= +k_1 \cdot [\text{HCOOH}] \cdot [\text{MeOH}] - k_{-1} \cdot [\text{H}_2\text{O}] \cdot [\text{HCOOMe}] + k_2 \cdot [\text{HCOOH}] \\ u \cdot \frac{d[\text{HCOOMe}]}{dz} &= +k_1 \cdot [\text{HCOOH}] \cdot [\text{MeOH}] - k_{-1} \cdot [\text{H}_2\text{O}] \cdot [\text{HCOOMe}] \\ u \cdot \frac{d[\text{CO}]}{dz} &= +k_2 \cdot [\text{HCOOH}] \end{aligned}$$

where  $k_{+1}$  is the kinetic constant of the forward reaction of esterification in  $\text{L}/(\text{mol} \cdot \text{s}^{-1})$ ,  $k_{-1}$  is the kinetic constant of the backward reaction of esterification in  $\text{L}/(\text{mol} \cdot \text{s}^{-1})$ ,  $k_2$  is the kinetic constant for the decomposition of the formic acid in  $1/\text{s}^{-1}$ ,  $[\text{HCOOH}]$  is the molar concentration of the formic acid,  $[\text{MeOH}]$  is the molar concentration of the methanol,  $[\text{HCOOMe}]$  is the molar concentration of the methyl formiate,  $[\text{H}_2\text{O}]$  is the molar concentration of water,  $[\text{CO}]$  is the molar concentration of carbon monoxide,  $u$  is the linear velocity of the fluid in  $\text{m}/\text{s}$ , and  $z$  the position in the tube in  $\text{m}$ .

Due to the decomposition reaction of formic acid, the assumptions about the monophasic system and a constant density are not respected. However, more complex models are not discussed here. The minimization of the error function between the model and the data is based on the Nelder-Mead method using the principle of the Simplex. The method works iteratively as described by Mathews and Fink.<sup>[10]</sup>

#### 5. Results and Discussion

The concentrations calculated with the online infrared spectrophotometer are based on a limited region of the spectra (between wavenumbers of  $450 \text{ cm}^{-1}$  and  $1'500 \text{ cm}^{-1}$ ). These values have been validated with Nuclear Magnetic Resonance (NMR) analysis. The measurement error is approximately 5% between the two methods. The points measured at approximately  $44 \text{ }^\circ\text{C}$  are used to determine the kinetics constants. The values are:  $k_{+1} = 2 \cdot 10^{-4} \text{ mol} \cdot \text{l}^{-1} \cdot \text{s}^{-1}$ ,  $k_{-1} = 5 \cdot 10^{-4} \text{ mol} \cdot \text{l}^{-1} \cdot \text{s}^{-1}$ , and  $k_2 = 3 \cdot 10^{-3} \text{ s}^{-1}$ . Fig. 2 shows the comparison between the measured data and the simulation based on the calculated kinetics constants. The observed difference between the measured data and the simulated data can be explained with the unexpected decomposition of formic acid. The proposed model does not include the two phase (gas/liquid) system. Fig. 3 presents a comparison between the batch reaction and the continuous reaction. The batch reaction is carried out in a glass vessel which prevents decomposition.

#### 6. Conclusion

This work highlights the role played by the metal-catalyzed decomposition of formic acid in the esterification reaction between formic acid and methanol. The continuous implementation of this reaction in an automated tubular microreactor provides estimates of the kinetic parameters. The precision of these estimates could be increased by measuring the concentrations at a wider range of flow rates. The proposed methodology provides a

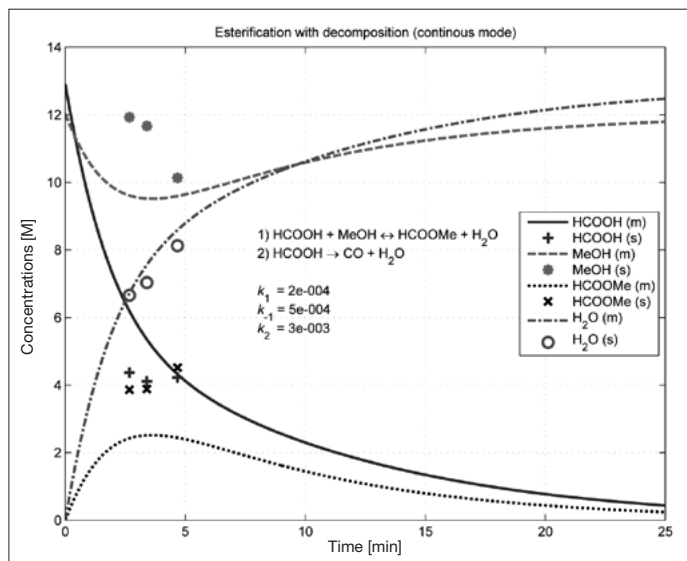


Fig. 2. Comparison between the measured data and the simulation for the esterification reaction in the tubular microreactor.

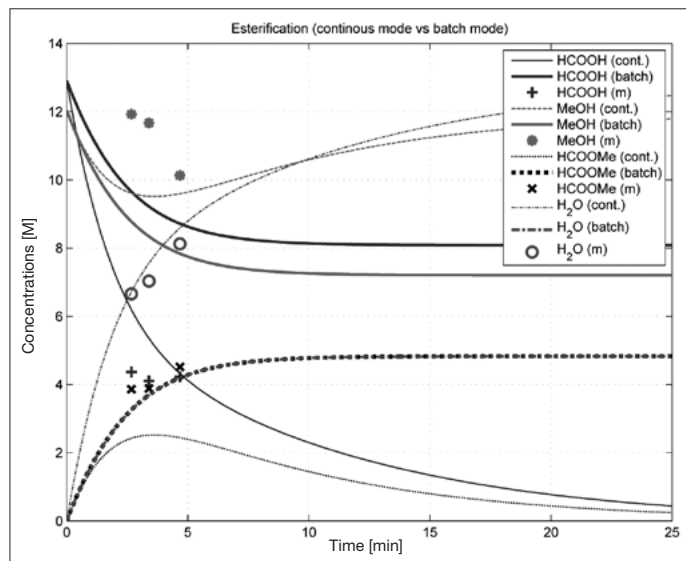


Fig. 3. Comparison between the esterification reactions carried out in a glass vessel (batch mode) and in the metal Ehrfeld reactor (continuous mode).

reaction screening platform that requires minimal personnel and material resources.

Received: October 24, 2010

- [1] O. Naef, *Chimia* **2007**, *61*, 672.  
 [2] M. Roch, Travail de Bachelor de l'école d'ingénieurs et d'architecte de Fribourg (filière de chimie), **2010**.  
 [3] B. Droz, Travail de Diplôme de l'école d'ingénieurs et d'architecte de Fribourg (filière de chimie), **2008**.  
 [4] L. Eriksson, E. Johansson, N. Kettaneh-Wold, C. Wikström, S. Wold, **2008**, Umetrics Academy.

- [5] B. Stuart, 'Infrared Spectroscopy: Fundamentals and Applications', **2004**, Wiley.  
 [6] R. G. Brereton, 'Applied Chemometrics for Scientists', **2007**, Wiley.  
 [7] G. Corminboeuf, M. Amrhein, O. Naef, *Chemometrics and Intelligent Laboratory Systems* **2007**, *86*, 168.  
 [8] R. Tauler, B. R. Kowalski, S. Flemming, *Anal. Chem.* **1993**, *65*, 2040.  
 [9] R. A. Kamarudin, N. A. Nordin, N. A. Buang, S. Ahmad, *Pertanika J. Sci. Technol.* **1998**, *6*, 71.  
 [10] J. H. Mathews, K. K. Fink, 'Numerical methods using Matlab', ed. 4, **2004**.