



# Performance evaluation of the Simtomax® CoronaCheck rapid diagnostic test

P.J. Ducrest<sup>a,\*,\*\*</sup>, A. Freymond<sup>b</sup>, J.-M. Segura<sup>b,\*</sup>

<sup>a</sup> GaDia SA, Route de l'île au bois 1A, 1870 Monthey, Switzerland

<sup>b</sup> Institute of Life Technologies - School of Engineering, HES-SO // University of Applied Sciences Western Switzerland, Sion, Switzerland

## ARTICLE INFO

### Keywords:

SARS-CoV-2

COVID-19

Serology

Rapid test

Lateral flow immunoassay

## ABSTRACT

The aim of this study was to evaluate the diagnostic performance of Simtomax® CoronaCheck, a serology rapid diagnostic test (RDT) for the detection of IgG and IgM against SARS-CoV-2. 48 plasma samples positive for SARS-CoV-2 based on RT-PCR and 98 negative control samples were studied. Diagnostic performance of the IgG/IgM RDT was assessed against RT-PCR and the electro-chemiluminescence immunoassay (ECLIA) Elecsys® Anti-SARS-CoV-2 total Ig. Overall, the RDT sensitivity was 92 % (95 % confidence interval [95 %CI]: 79–97), specificity 97 % (95 % CI: 91–99 %), PPV 94 % (95 % CI: 81–98) and the NPV 96 % (95 % CI: 89–99). When considering only samples collected  $\geq 15$  days post-symptoms (DPS), the sensitivity increased to 98 % (95 %CI: 86–100) and the specificity was 97 % (95 % CI: 91–99 %). Two samples with 180 DPS were still positive for IgG. Globally, this IgG/IgM RDT displayed a high diagnostic accuracy for SARS-CoV-2 IgG/IgM detection in plasma samples in high COVID-19 prevalence settings. It could be effectively used, in absence of facilities for routine diagnostic serology, for samples with a DPS between 15 and 180 days.

## 1. Introduction

SARS-CoV-2 is the etiological agent of a severe pneumonia first reported in Wuhan (Hubei, China), called 2019 Coronavirus Disease (COVID-19). Protein sequence analysis of seven proteins showed that the virus is related to the Severe Acute Respiratory Syndrome Coronavirus (SARS-CoV) and the Middle East Respiratory Syndrome Coronavirus (MERS-CoV) with similar epidemiology (Kannan et al., 2020; Zhou et al., 2020). Currently, the detection method for SARS-CoV-2 is based on viral RNA detection using Reverse-Transcription PCR (RT-PCR) but other tests such as chest computed tomography (CT) imaging or antigen/antibody testing can also be used (Li et al., 2020a,b). Serological analysis may be applied to detect past exposure to the virus and possibly if a patient has developed immunity against the virus. It is widely accepted that IgM provides the first line of defense during acute viral infections, prior to the generation of adaptive, high affinity IgG responses that are important for long term immunity and immunological memory (Li et al., 2020b). Several authors analyzed the antibody kinetics in COVID-19 patients. Zhao et al. (2020) showed that among 173 patients, the seroconversion sequentially appeared for total antibody,

IgM and then IgG, with a median time of 11, 12 and 14 days after symptom onset. The majority of antibodies are produced against the most abundant protein of the virus, which is the nucleocapsid protein (NP). Therefore, serological tests that detect antibodies to NP should be the most sensitive. In addition, because the receptor-binding domain of the Spike protein (RBD-S) is the host attachment protein, antibodies against RBD-S should be very specific. Therefore, according to some authors, using one or both antigens should result in high sensitivity and specificity (Sethuraman et al., 2020). The rapid diagnostic test (RDT) Simtomax® CoronaCheck developed by Augurix SA (Switzerland) uses both antigens as described in To et al. (2020). The gold nanoparticles used for detection are conjugated with SARS-CoV-2 Receptor Binding Domain and Nucleocapsid protein with the aim to specifically bind IgM and/or IgG in COVID-19 positive samples. A recent clinical evaluation of Augurix RDT at the University Hospitals of Geneva and Lausanne (Switzerland) demonstrated high diagnostic accuracy for IgG in whole-blood, plasma and sera samples (Andrey et al., 2020; Coste et al., 2021).

The aim of this study was to evaluate the performance of this RDT with plasma samples in a high COVID-19 prevalence setting using as

\* Corresponding author at: Institute of Life Technologies - School of Engineering, HES-SO // University of Applied Sciences Western Switzerland, 1950 Sion, Switzerland.

\*\* Corresponding author.

E-mail addresses: [percevent.ducrest@gadia.net](mailto:percevent.ducrest@gadia.net) (P.J. Ducrest), [jmanuel.segura@hevs.ch](mailto:jmanuel.segura@hevs.ch) (J.-M. Segura).

<https://doi.org/10.1016/j.jviromet.2021.114178>

Received 27 October 2020; Received in revised form 19 April 2021; Accepted 30 April 2021

Available online 4 May 2021

0166-0934/© 2021 The Author(s).

Published by Elsevier B.V. This is an open access article under the CC BY-NC-ND license

(<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

reference methods RT-PCR and an Electro-chemiluminescence immunoassay (ECLIA) Elecsys® Anti-SARS-CoV-2 total Ig (Roche, Switzerland).

## 2. Materials & methods

### 2.1. Study population and blood sample collection

Forty-eight anonymized remaining patients' plasma-EDTA specimens, supplied by INO Specimens BioBank, ISB (Clermont-Ferrand, France), were used for this method evaluation (Fig. 1). Only laboratory-based information was used in this study. All 48 samples were from patients positive for SARS-CoV-2 based on RT-PCR measurements on nasopharyngeal swab samples using the BD SARS-CoV-2 reagent kit for the BD Max system (Becton Dickinson and Co, US). The RT-PCR analysis were performed by INO Specimens. The median CT value was 25.6 (IQR 20.05–29.15). The plasma-EDTA specimens (n = 48) were all collected at days post symptom (DPS) of at least 10 days. A proportion of 48 % (23/48) of the plasma-EDTA specimens were additionally tested for total immunoglobulin against COVID-19 with an electro-chemiluminescence immunoassay (ECLIA) at INO Specimens BioBank (Fig. 1). As negative controls, anonymized unmatched control plasma samples (n = 98), supplied by AbBaltis (Kent, UK) with a collection date before 2018, were used (Fig. 1).

### 2.2. Augurix IgM/IgG immunochromatographic rapid test

Commercial CE-labeled SARS-CoV-2 IgM/IgG RDT were from Augurix (Switzerland). This test detects IgG and IgM against NP and RBD-S antigens and can be used either with capillary blood, whole blood, plasma or serum. One IgM/IgG rapid test per sample was used. Following manufacturers' instructions, 10 µL of plasma were applied for each sample. IgG and IgM responses were read after 15 min following manufacturer's instructions, blinded to the reference method results. The tests were considered COVID-19 positive if either the IgM line or the IgG line or both lines were positive.

### 2.3. Electro-chemiluminescence immunoassay Elecsys® Anti-SARS-CoV-2 total Ig

ECLIA experiments were performed at INO Specimens Biobank. Elecsys® Anti-SARS-CoV-2 total Ig (Roche, Switzerland) makes use of the nucleocapsid protein of SARS-CoV-2 as antigen. This test detects the total Ig against NP antigen. Total Ig was analyzed according to manufacturer's instructions. The assays were run on a Cobas e 601 (Roche, Switzerland) according to manufacturer's protocol. Positivity was

defined by the manufacturer as a cut-off index (COI)  $\geq 1.0$ .

### 2.4. Study end points

The primary end point was to assess the accuracy of IgG/IgM detection in plasma using Augurix IgM/IgG RDT against the RT-PCR reference method, within a cohort of 48 RT-PCR confirmed COVID-19, with day post-symptoms (DPS) of  $\geq 10$  days, and 98 control plasma samples. The secondary end point was to assess Augurix IgG/IgM RDT performance against Electro-chemiluminescence immunoassay (ECLIA), Elecsys® Anti-SARS-CoV-2 total Ig (Roche, Switzerland).

### 2.5. Statistics

Vassarstats online tool ([www.vassarstats.net](http://www.vassarstats.net)) was used to calculate sensitivity (SE), specificity (SP), positive and negative predictive values (PPV, NPV), 95 % confidence intervals, median, Interquartile range (IQR) and Cohen's kappa values. Significance (p-values) were calculated using a Mann-Whitney U test. Statistical significance was defined as  $p < 0.05$ .

## 3. Results

### 3.1. Baseline characteristics

The demographic characteristics of patients' samples were as follows: the 48 COVID-19-positive samples were from patients older (median = 49 years old, IQR 33–58.75) compared to the healthy patients (n = 98) (median = 34.5 years old, IQR 18–44.75;  $p < 0.05$ ). The proportion of females was 56 % (n = 20) and 51 % (n = 50) in the COVID-19 positive and in the healthy control group, respectively.

Among the COVID-19 samples, the median delay between symptom onset and sampling was 21 days (IQR 16–32 days), but not less than 10 days. The longest DPS (one single sample) was 180 days.

A detailed description of all the available information on the samples and the results of the various tests is provided in the supplementary information.

### 3.2. Specificity of IgG/IgM RDT on the negative control group


The diagnostic specificity of the IgG/IgM RDT was assessed on the COVID-19 negative control group with a sampling date before 2018 (n = 98). The results are shown in Tables 1 and 2. IgG/IgM RDT results were negative in 96.9 % (95/98) of the cases (95 %CI: 91–100 %). Three discordant results showed a positive IgM line while negative with RT-PCR (false positives compared to RT-PCR results). The specificity (SP) of the IgG/IgM RDT was therefore 97 % (95 % CI: 91–99 %).

**Table 1**

Diagnostic performance of Simtomax CoronaCheck RDT compared to RT-PCR as reference method for different sample groups.

	SE % (95 % CI)	SP % (95 % CI)	PPV % (95 % CI)	NPV % (95 % CI)
<b>All samples (n = 146); Prevalence = 48/146 = 33 %</b>				
<b>IgG/IgM RDT vs RT-PCR</b>	92 (79–97)	97 (91–99)	94 (81–98)	96 (89–99)
<b>Samples with DPS &lt; 15 and negative controls (n = 105); Prevalence = 7/105 = 6.7 %</b>				
<b>IgG/IgM RDT vs RT-PCR</b>	57 (20–88)	97 (91–99)	57 (20–88)	97 (91–99)
<b>Samples with DPS <math>\geq 15</math> DPS and negative controls (n = 139); Prevalence = 41/139 = 29 %</b>				
<b>IgG/IgM RDT vs RT-PCR</b>	98 (86–100)	97 (91–99)	93 (80–98)	99 (94–100)

RDT: Simtomax CoronaCheck rapid diagnostic test; SE: sensibility; SP: specificity; PPV: positive predictive value; NPV: negative predictive value; ECLIA: Electro-chemiluminescence immunoassay.

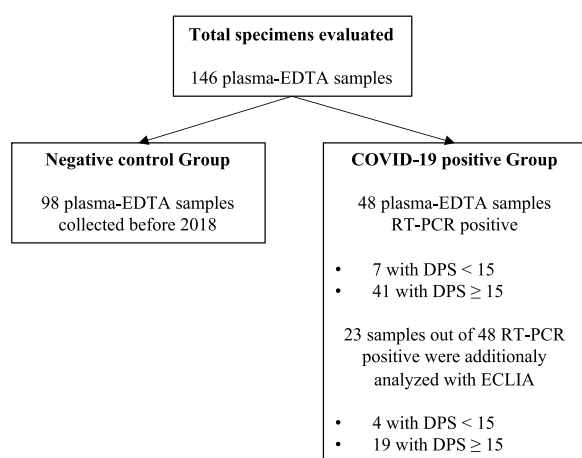

**Fig. 1.** Description of the plasma samples used in this study.

**Table 2**

Diagnostic performance of Simtomax CoronaCheck RDT compared to ECLIA total Ig as reference method for different sample groups.

	SE % (95 % CI)	SP % (95 % CI)	PPV % (95 % CI)	NPV % (95 % CI)
<b>All samples (n = 121); Prevalence = 23/121 = 19 %</b>				
<b>IgG/IgM RDT vs ECLIA</b>	91 (70–98)	97 (91–99)	88 (67–97)	98 (92–100)
<b>Samples with DPS &lt; 15 and negative controls (n = 102); Prevalence = 4/102 = 3.9 %</b>				
<b>IgG/IgM RDT vs ECLIA</b>	50 (9–91)	97 (91–99)	40 (7–83)	98 (92–100)
<b>Samples with DPS ≥ 15 DPS and negative controls (n = 117); Prevalence = 19/117 = 16 %</b>				
<b>IgG/IgM RDT vs ECLIA</b>	100 (79–100)	97 (91–99)	86 (64–96)	100 (95–100)

### 3.3. Sensitivity of IgG/IgM RDT on RT-PCR confirmed COVID-19 samples

IgG/IgM RDT diagnostic sensitivity was assessed on the 48 samples positive for COVID-19 based on RT-PCR. The results are shown in Table 1. Both methods revealed similar results in 91.7 % (44/48) of the samples (95 % CI: 79–97 %). Four discordant results showed a negative result with the IgG/IgM RDT both for IgG and IgM (no line observed) while being positive with RT-PCR (false negatives compared to RT-PCR). The resulting sensitivity (SE) of the IgG/IgM RDT was 92 % (44/48) (95 % CI: 79–97), while the positive predictive value (PPV; using a prevalence of 48/146 = 33 %) was 94 % (44/47) (95 % CI: 81–98) and the negative predictive value (NPV) 96 % (95/99) (95 % CI: 89–99).

As shown in Table 1, most false-negative results (3 out of 4) exhibited a DPS between 10 and 15. Only one false-negative result was observed with a DPS ≥ 15. When taking into account exclusively the results in the ≥ 15 DPS group, the IgG/IgM RDT sensitivity (SE) was 98 % (40/41) (95 % CI: 86–100), while the PPV (using a prevalence of 41/139 = 29 %) was 93 % (40/43) (95 % CI: 80–98) and the NPV 99 % (95/96) (95 % CI: 94–100). It is remarkable that two samples with days post symptoms (DPS) of respectively 170 and 180 days were still positive for IgG (Sup. Information).

### 3.4. Sensitivity of IgG/IgM RDT with an electro-chemiluminescence immunoassay as reference method

The accuracy of the IgG/IgM RDT was also assessed using an electro-chemiluminescence immunoassay (ECLIA), Elecsys® Anti-SARS-CoV-2 total Ig, as reference. ECLIA was conducted on a random selection of 23 out of the 48 COVID-19 positive samples based on RT-PCR. The median cut-off index (COI) was 63.4 (IQR 5–85 COI). The COI was not significant higher in the ≥ 15 DPS group (76.9; IQR 5.8–86) compared to the < 15 DPS group (26.3; IQR 1–49.5;  $p = 0.384$ ). This might be at least partly attributed to the small sample size of the < 15 DPS group ( $n = 4$ ). The results obtained using the IgG/IgM RDT on the 23 samples are shown in Table 2. Both methods yielded similar results in 91.3 % (21/23) of the cases (95 % CI: 70–98 %). Two discordant results showed an IgG/IgM RDT negative result, both for IgG and IgM, while were positive by ECLIA (false negatives). This resulted in an IgG/IgM RDT sensitivity (SE) of 91 % (21/23) (95 % CI: 70–98), while the PPV (using a prevalence of 23/121 = 19 %) was 88 % (21/24) (95 % CI: 67–97) and the NPV 98 % (95/97) (95 % CI: 92–100) compared to ECLIA.

The two false-negative results exhibited a DPS between 10 and 15. When using exclusively the results in the ≥ 15 DPS group, there was a complete agreement between the results of the IgG/IgM RDT and ECLIA. In this case, the IgG/IgM RDT sensitivity (SE) was therefore 100 % (19/19) (95 % CI: 79–100), while the PPV was 86 % (19/22) (95 % CI: 64–96) and the NPV 100 % (95/95) (95 % CI: 95–100).

## 4. Discussion

The main finding of this evaluation study, using an unmatched case-control design including 67.1 % (98/146) of negative control samples, is that the diagnostic accuracy of IgG/IgM Augurix RDT on plasma samples when compared to RT-PCR confirmed cases displayed a SE of 92 %, a SP of 97 %, a PPV of 94 % and a NPV of 96 %. When compared to ECLIA positive samples, the diagnostic accuracy of IgG/IgM Augurix RDT displayed a SE of 91 %, a SP of 97 %, a PPV of 88 % and a NPV of 98 %. The sensitivity (SE) of IgG/IgM Augurix RDT was not significantly different for both reference methods ( $p = 0.756$ ) with strong Cohen's kappa correlations of 89 % for RDT vs RT-PCR and 87 % for RDT vs ECLIA. The diagnostic accuracy of the RDT further increased when analyses were performed exclusively on samples collected after 15 DPS and exhibited excellent sensitivity (98 %) and NPV (99 %). For samples collected within a DPS < 15 days, the diagnostic performance was clearly poorer with 57 %, 97 %, 57 % and 97 % for SE, SP, PPV and NPV, respectively.

It is interesting to notice that the two false-negative results obtained with Augurix RDT corresponded to borderline samples in ECLIA (Cut-off index of 1.43 and 1.19) with a DPS between 10 and 15 days. The ECLIA manufacturer defines positive samples when the cut-off index (COI) value is ≥ 1.0. This finding indicates that the analytical sensitivity of Augurix RDT is lower than the ECLIA Elecsys® Anti-SARS-CoV-2 total Ig (Roche, Switzerland) and that insufficient analytical sensitivity might at least partly explain the poor performance of the RDT test at DPS < 15 days.

For samples with DPS > 15, there is a perfect agreement between ECLIA and Augurix RDT, which can be explained by the fact that both assays target the immune response against the full-length N protein of SARS-CoV-2. The overall good specificity of the Augurix RDT might be offered by the fact that it also targets the immune response against the Receptor binding domain (RBD) of S protein.

The overall performance, in particular for DPS > 15, indicates that Augurix RDT could be fit for purpose in clinical settings where a high prevalence of COVID-19 prevails, especially in situations where ECLIA is not available. Diagnostic performance in low prevalence populations still needs to be experimentally determined and it would be interesting to validate the results on larger populations. The results of our study on plasma samples are similar with those recently published on whole blood and plasma samples, which indicated a sensitivity of Augurix RDT between 93 % and 100 % for samples with a DPS of >15 days (Andrey et al., 2020; Coste et al., 2021), but differ from prior studies using Augurix and other RDTs that observed a lower sensitivity of 56.4 % for a DPS of > 21 days (Rudolf et al., 2020). However, differences in methodology and sample size between the two studies make a comparison difficult. Concerning the specificity of the test, the excellent performance observed in this study is in line with the results of preceding publications (Andrey et al., 2020; Coste et al., 2021). Three control blood samples turned out to be IgM positive by RDT although they were collected before 2018. Non-specific binding of undefined IgM antibodies in the samples with the antigens present on the IgM line might possibly explain this finding. But overall, Augurix RDT might be a suitable choice in situations where a high PPV is instrumental.

The second notable finding of this study lies in the fact that IgG seropositivity is still present 180 days after symptom onset in spite of normal antibody decline (Long et al., 2020; Seow et al., 2020). To our knowledge, it is the first time that SARS-CoV-2 IgG seropositivity is demonstrated with RDT 180 DPS. The present study indicates also that a certain level of SARS-CoV-2 IgG is present constantly with a concentration sufficient to be detectable with RDT, from 15 days to at least 180 days post symptoms. This finding applies to the Augurix RDT and cannot be generalized to other RDTs for SARS-CoV-2 specific antibodies currently available. It would be interesting to quantitatively determine the level of IgG/IgM 180 days post symptoms onset to confirm this finding obtained with a qualitative assay.

In addition, the test provided clear results without indeterminate or

invalid measurements. There are however several limitations to this study. First, we present here the results of a method evaluation study and not a seroprevalence study. Therefore, the PPV obtained here (based on a 32.9 % proportion of cases defined as laboratory confirmed SARS-CoV-2 by RT-PCR) will be lower in a low prevalence setting, e.g. when testing the asymptomatic population. Another limitation of this validation study lies in the limited sample size leading to broad 95 % confidence intervals, requiring confirmation of these data at a larger scale. Also, here we used plasma and the test was performed in a laboratory environment; we may expect different results in real-life at patients' bed and using capillary blood. Finally, our present conclusions only apply to the Augurix RDT, and must not be generalized to other currently available RDTs for SARS-CoV-2 specific antibodies.

In conclusion, Augurix RDT is not meant to replace a SARS-CoV-2 RT-PCR diagnostic test in the first week of the disease, but could be a reliable option for assessing the SARS-CoV-2 serology in moderate to high COVID-19 prevalence settings, i.e. when testing the sub-population of individuals having presented COVID-19 symptoms, especially in situations where automated ECLIA or ELISA are not available, with samples collected between at least 15 days and up to 180 days after the onset of symptoms.

## Contributions

**Percevent J Ducrest:** Conceptualization, Methodology, Investigation, Formal analysis, Writing - Original Draft preparation. **Antoine Freymond:** Investigation, Formal analysis, Writing - Original Draft preparation. **Jean-Manuel Segura:** Writing - Original Draft preparation, Writing - Review & Editing preparation, Visualization

## Ethical consideration

This study was evaluated by the Ethics Committee of Canton de Vaud, Lausanne, Switzerland (CER-VD) and they judged that it did not deserve a specific approval being only a quality assessment of diagnostic tests with foreign residual samples.

All necessary patient/participant consent has been obtained by the supplier of residual samples and the appropriate institutional forms have been archived.

## Funding

This research was financially supported by the HES-SO Valais-Wallis.

## Declaration of Competing Interest

Percevent J Ducrest has a R&D mandate with Augurix SA, the

manufacturer of the RDT used in this study. Augurix SA had no role in the study design, the realization nor in result interpretation. The other authors have no conflict of interest to disclose.

## Acknowledgments

We thank Augurix SA (Monthey, Switzerland) for providing Simto-max CoronaCheck RDTs free-of-charge.

## Appendix A. Supplementary data

Supplementary material related to this article can be found, in the online version, at doi:<https://doi.org/10.1016/j.jviromet.2021.114178>.

## References

- Andrey, D.O., Cohen, P., Meyer, B., et al., 2020. Diagnostic accuracy of Augurix COVID-19 IgG serology rapid test. *Eur. J. Clin. Invest.* 50, e13357 <https://doi.org/10.1111/eci.13357>.
- Coste, A.T., Jaton, K., Papadimitriou-Oliveris, M., Greub, G., Croxatto, A., 2020. Comparison of SARS-CoV-2 serological tests with different antigen targets. *J. Clinical. Virol.* 134, 104690 <https://doi.org/10.1016/j.jcv.2020.104690>.
- Kannan, S., Shaik Syed Ali, P., Sheeza, A., Hemalatha, K., 2020. COVID-19 (Novel Coronavirus 2019) – recent trends. *Eur. Rev. Med. Pharmacol. Sci.* 24, 2006–2011. <https://doi.org/10.26355/eurev.202002.20378>.
- Li, C., Zhao, C., Bao, J., Tang, B., Wang, Y., Gu, B., 2020a. Laboratory diagnosis of coronavirus disease-2019 (COVID-19). *Clin. Chim. Acta* 510, 35–46. <https://doi.org/10.1016/j.cca.2020.06.045>.
- Li, Z., Yi, Y., Luo, X., et al., 2020b. Development and clinical application of a rapid IgM-IgG combined antibody test for SARS-CoV-2 infection diagnosis. *J. Med. Virol.* 92, 1518–1524. <https://doi.org/10.1002/jmv.25727>.
- Long, Q., Liu, B., Deng, H., et al., 2020. Antibody responses to SARS-CoV-2 in patients with COVID-19. *Nat. Med.* 26, 845–848. <https://doi.org/10.1038/s41591-020-0897-1>.
- Rudolf, F., Kaltenbach, H.M., Linnik, J., Ruf, M.T., Niederhauser, C., Nickel, B., Gyax, D., Savic, M., 2020. Clinical characterization of eleven lateral flow assays for detection of COVID-19 antibodies in a population. *medRxiv*. <https://doi.org/10.1101/2020.08.18.20177204>, 2020.08.18.20177204.
- Seow, J., Graham, C., Merrick, B., et al., 2020. Longitudinal evaluation and decline of antibody responses in SARS-CoV-2 infection. *Nat. Microbiol.* 5, 1598–1607. <https://doi.org/10.1038/s41564-020-00813-8>.
- Sethuraman, N., Jeremiah, S.S., Ryo, A., 2020. Interpreting diagnostic tests for SARS-CoV-2. *JAMA* 323 (22), 2249–2251. <https://doi.org/10.1001/jama.2020.8259>.
- To, K.K.W., et al., 2020. Temporal profiles of viral load in posterior oropharyngeal saliva samples and serum antibody responses during infection by SARS-CoV-2: an observational cohort study. *Lancet Infect. Dis.* 20, 565–574. [https://doi.org/10.1016/S1473-3099\(20\)30196-1](https://doi.org/10.1016/S1473-3099(20)30196-1).
- Zhao, J., Yuan, Q., Wang, H., Liu, W., et al., 2020. Antibody responses to SARS-CoV-2 in patients with novel coronavirus disease. *Clin. Infect. Dis.* 344 <https://doi.org/10.1093/cid/ciaa344> ciaa.
- Zhou, P., Yang, X., Wang, X., et al., 2020. Pneumonia outbreak associated with a new coronavirus of probable bat origin. *Nature* 579, 270–273. <https://doi.org/10.1038/s41586-020-2012-7>.